

# Nephros EndoPur Endotoxin Filter (Flat) - Instructions for Use

## INTRODUCTION

Information on this sheet must be read before the use of this device to ensure safe and effective operation in a clinical or hospital environment.

**Recommended Storage:** Between 5 and 35°C (41 and 95°F).

## INDICATIONS

**Intended Use:** The EndoPur Endotoxin Filter (Flat) is a hollow fiber ultrafilter that retains bacteria and endotoxin from fluid.

**Indications for Use:** The EndoPur Endotoxin Filter intended use is to filter water used with hemodialysis devices. It assists in providing hemodialysis quality water. The device is not a complete water treatment system, but serves to remove biological contaminants. Therefore it must be used in conjunction with other water treatment equipment (Reverse Osmosis, Deionization, etc.).

**Use Life:** The device is intended for continuous use up to one year. Once it completes its useful life or maximum number of disinfection cycles, the filter should be replaced and discarded. Do not attempt to sterilize or reuse it.

**Location:** Due to its size and flow capacity, the EndoPur Endotoxin Filter should be installed as part of the dialysis water distribution loop after the Reverse Osmosis (or Deionization) treatment system in a clinical environment.

To achieve the desired flow rate needed for the distribution loop, it may be necessary to install multiple filters in appropriate filter sizes. Install one or more branch tees to run multiple filters in parallel.

## WARNINGS & PRECAUTIONS

**Caution:** When used as a medical device, federal law (USA) restricts this device to sale by or on the order of a physician.

**Pressure:** The EndoPur Endotoxin Filter is intended for a maximum differential water pressure of 30 psi (2 bar).

**Replacement:** It is recommended to establish a regular maintenance schedule for replacing the filter. The filter should be replaced when the maximum differential pressure of 30 psi (2 bar) is exceeded or the maximum disinfection cycles are reached.

## FILTER INSTALLATION & REMOVAL

**New Install:** If it is the first time a reusable housing is being installed with an endotoxin retentive filter, refer to the *Housing Installation* section before proceeding with the instruction below.

**Note:** Personnel installing filters must be properly trained per this IFU.

- Wash hands and place on clean disposable gloves.
- Turn off the fluid source upstream of the filter and vent any excess pressure from the housing via its bleed valve or outlet test valve.
- Remove the housing bowl/cover, remove the old filter, and discard per facility protocol.
- Wash and sanitize hands and place on clean disposable gloves.
- Open a new EndoPur Endotoxin Filter blister pack and aseptically remove the filter.
- Insert the O-ring end of the filter into the head of the housing. It may be necessary to use a twisting motion to ensure that the filter is firmly in place and the O-rings seat properly.
- Re-attach the housing bowl/cover.
- Open the bleed valve located at the top of the housing cap to fully purge the air from inside the housing/bowl. All air must be fully purged from the filter bowl/housing at this time to achieve sufficient flow rates.

- Open the upstream fluid source and prime the new filter by opening the outlet test valve. Purge it of any additional trapped air for 3-5 minutes.
- Close the outlet test valve and bleed valve, dry housing of any fluid from purging and verify the housing and cover are properly sealed.

## OPERATION & DISINFECTION

- After installation of a new filter, it is recommended to disinfect the system as per standard clinic procedure.
- The EndoPur Endotoxin Filter is compatible with the following disinfection cycles with no degradation in safety or efficacy:

Disinfection Method	Maximum Cycles <sup>1</sup>
1% MinnCare	52
1% Bleach	52
Hot Water ≤ 85°C <sup>2,3</sup>	52

**Note:** 1. When the filter completes its useful life or maximum number of disinfection cycles it should be replaced and discarded.

2. Based on cycles of 1.5-2 hour ramp to 85°C, followed by 2 hour hold at 85°C, 1-1.5 hour cool down to room temperature, and a maximum differential pressure of 8psi at 85°C.

3. Hot water disinfection is only applicable to products with a part numbers ending in a letter "H" (70-0110H & 70-0120H).

- Disinfection should be carried out as per standard clinic procedures. No special precautions or procedures are required for disinfection and the filter should be treated as an extension of the distribution system.
- Following chemical disinfection the fluid must be tested for residual disinfectant per standard procedure. Verification in absence of chemical residuals are required to proceed.
- Continue to rinse the EndoPur Endotoxin Filter until verifying the absence of chemical residuals as required per clinic procedures.
- Pressure drop across the EndoPur Endotoxin Filter maybe higher than a typical endotoxin filter. This increase in pressure is due to a tighter membrane pore size. The EndoPur Filter should not provide any noticeable flow velocity reduction during standard operation.
- The filter should be replaced and discarded when maximum differential pressure of 30 psi (2 bar) is exceeded.


## INTEGRITY TESTING

**Note:** If multiple filters are installed (as shown in Diagram B: *Parallel Housing and Filter Installation*) only one filter can be tested at a time and must be isolated using the filter isolation valve leading to all other filters. Once the filter is isolated, follow the instructions below

- The filter integrity can be verified with a pressure holding test after the filter has been properly installed, connected, and primed.
- Turn off the fluid source valve and open the inlet test valve to bleed off any residual pressure.
- A pressure gauge must be installed to monitor the inlet filter pressure in order to carry out this test. Connect an air source (compressed air or air pump) to the inlet test port as shown in *Housing and Filter Installation Example*.
- Do not exceed 30 psi to prevent damage to the filter membrane.
- Open outlet test valve, ensure that the inlet test valve is open, and pressurize the filter inlet; ensure the outlet test port is venting. Raise the air pressure to 15 psi at the filter inlet and allow water to exit from the outlet test port.

# Nephros EndoPur Endotoxin Filter (Flat) - Instructions for Use

- When water stops flowing from the outlet test port, close the outlet test valve and check for external leaks via pressure gauge.
- Open the outlet test valve and re-pressurize as necessary to reach 15 psi at the filter inlet.
- With the outlet test valve open, close the inlet test valve and allow the pressure to stabilize for 10 seconds.
- Monitor the pressure gauge and determine the pressure drop for a period of 1 minute.
- If the pressure drops by more than 1 psi over a minute, check for leaks and repeat the test to confirm. If the filter fails, it must be replaced.
- Close the outlet test valve and remove air source. Open fluid source valve, purge air out of the housing/bowl using the bleed valve, and re-prime filter to return to operation.

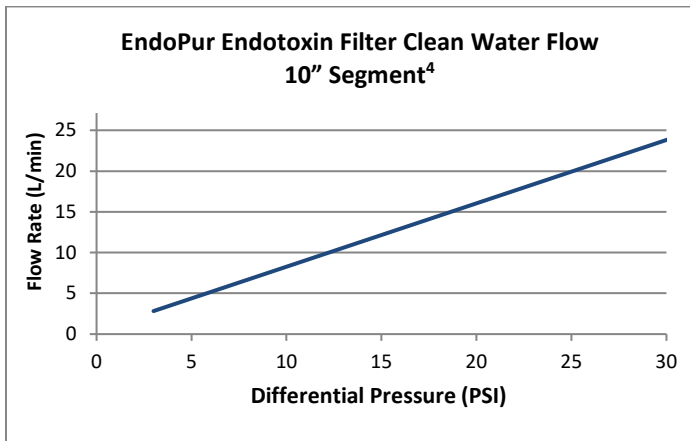

Note 4: Maximum Flow Rate per 10" Segment = 2.5 GPM

Specifications	EndoPur Endotoxin Filter
Max Differential Pressure	30 psi (2 bar)
Filter Membrane	Medisulfone <sup>®</sup>
Material	Polysulfone
MW cut-off	15 kDa
Bacterial Retention	> 10 <sup>11</sup> (B. diminuta)
Virus Retention	>10 <sup>8</sup> (PhiX-174)
Endotoxin Retention	> 10 <sup>5</sup> EU/ml
Expected Life	Up to 1 year

Medisulfone<sup>®</sup> is a registered trademark of Medica S.p.A.

## HOUSING INSTALLATION


If no endotoxin retentive cartridge filter housings are currently installed, the initial install of the EndoPur Endotoxin Filter requires tapping into an existing section of the line between the fluid source and the distribution loop.

**Note:** EndoPur Endotoxin Filter is only to be installed in reusable cartridge filter housings that comply with AAMI/ANSI/ISO 26722 for material compatibility (or made from 316 Stainless Steel or made from pure polypropylene with no fillers, colorants, plasticizers or lubricants) and accepts 10", 20", or 30" 222 O-ring head cartridge filters.

A spacer may be required for longer housings to properly seat both O-rings and minimize the dead space areas. Contact Nephros for acceptable spacers.


Examples of standard installations with a single and multiple EndoPur Endotoxin Filters with cartridge housings are shown in Diagrams (A) and (B) below. Bleed valves are not shown.

### A) Single Housing and Filter Installation

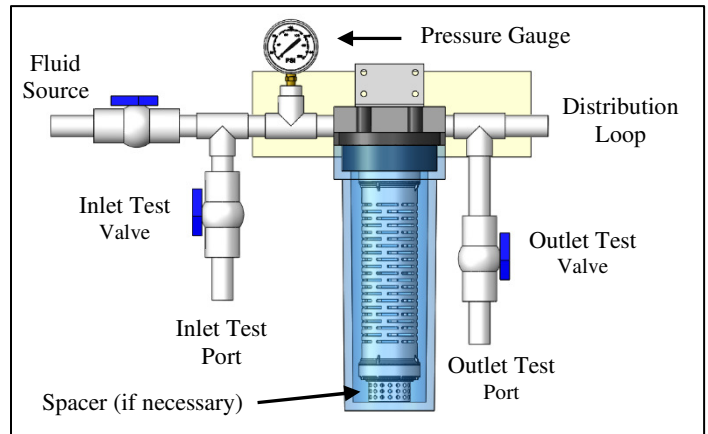

For higher flow rates to be achieved, multiple housings may need to be installed in parallel as shown in Diagram B.

### B) Parallel Housing and Filter Installation

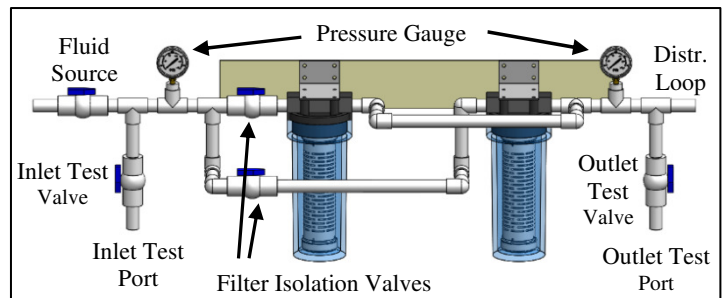

## Manufacturer:

Nephros, Inc.  
380 Lackawanna Place  
South Orange, NJ 07079 USA  
833-NEPHROS